




In today's dynamic non-critical care environment, workloads are compressed, patient acuity fluctuates and the nursing shortage is often keenly felt. These factors, combined with a lack of real-time monitoring for non-critical patients, are contributing to increased patient risk and unexpected in-hospital mortality.


NURSES HAVE MORE TO DO & LESS TIME TO DO IT

With an increase in patient complexity and variability, nurses face the mounting challenge of documenting and leveraging timely, accurate data to make informed care decisions.

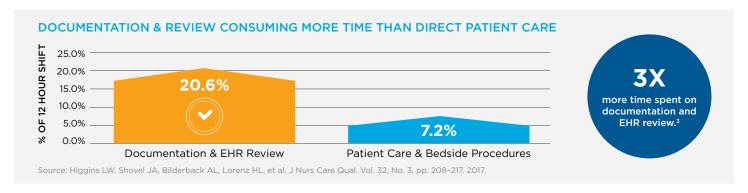

THE COST OF ERRORS & DELAYED RECOGNITION

Despite steady improvement in hospital care and initiatives to reduce harm for patients, medical error rates are significantly higher in the U.S. compared with other developed countries,^{4,5} and are the third-leading cause of death in this country.⁶

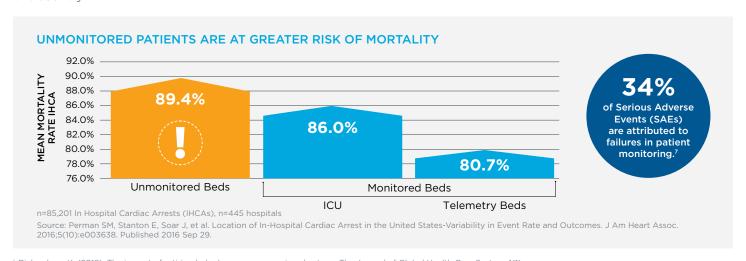

- Richardson, K. (2018). The impact of retiring baby boomers on nursing shortage. The Journal of Global Health Care System, 1(1).
- ² Brown H, Terrence J, Vasquez P, et al. Continuous monitoring in an inpatient medical-surgical unit: a controlled clinical trial. Am J Med 2014; 127:226-232
- ³ Higgins LW, Shovel JA, Bilderback AL, Lorenz HL, et al. J Nurs Care Qual. Vol. 32, No. 3, pp. 208-217. 2017.
- ⁴ Anderson JG, Abrahamson K.Your Health Care May Kill You: Medical Errors. Study Health Technol Inform. 2017;234:13-17.
- $^{\rm 5}$ Risk factors for patient-reported medical errors in eleven countries. Health Expect. 2014 Jun; 17(3): 321–331
- ⁶ Makary M A, Daniel M. Medical error—the third leading cause of death in the US BMJ 2016; 353:i2139
- ⁷ van Galen LS, Struik PW, Driesen BE, et al. Delayed Recognition of Deterioration of Patients in General Wards Is Mostly Caused by Human Related Monitoring Failures: A Root Cause Analysis of Unplanned ICU Admissions. PLoS One. 2016;11(8):e0161393. Published 2016 Aug 18. doi:10.1371/journal.pone.0161393

MOVING FROM EPISODIC MONITORING TO ENHANCED SURVEILLANCE

Capsule Vitals Plus delivers intelligence to the point of care, setting a new standard for efficiency, safety and patient experience. Leveraging Capsule's industry-leading connectivity management, Vitals Plus enables hospitals to securely collect, analyze and integrate a range of patient information at the bedside. Clinicians get access to real-time vitals data, captured and charted automatically, along with contextual information to inform care decisions.

A NEW LEVEL OF WORKFLOW EFFICIENCY & CONVENIENCE

- · Reduces charting time from hours to minutes, so nurses can spend more time with patients
- · A single screen for login, patient association, vitals monitoring and charting of 15 elements, improving workflow
- · Ability to see a patient-centric view of 72 hours of vital signs history, right at the bedside

IMPROVES PATIENT SAFETY & CARE

- Eliminates risks associated with manual transcription errors and data/chart mix-ups
- · Rapid authenticatoin gives clinicians easy access to patient data at the bedside
- · Lets users validate data directly at the bedside, enabling timely care decisions
- · Role-based authorization ensures the right data is entered by the right team member

CUSTOMIZABLE TO MEET YOUR NEEDS

- Three monitoring modes: spot-check, intervals, continuous
- Supports both Masimo SET® and Nellcor™ OxiMax™ pulse oximetry
- Supports both FILAC™ 3000 oral/axillary and Exergen TAT-5000S TemporalScanner™
- Added modifiers and custom fields to meet unique patient needs


CONSOLIDATED VITALS CAPTURE & ANALYSIS ON A SINGLE SCREEN



- Simplified clinical documentation with validation from the bedside
- Highly usable single screen for vital signs and charting
- 72 hours of patient vital signs across all devices
- Rapid authentication with secure patient association



ADVANCED FUNCTIONALITY FOR INCREASED SAFETY & WORKFLOW EFFICIENCY

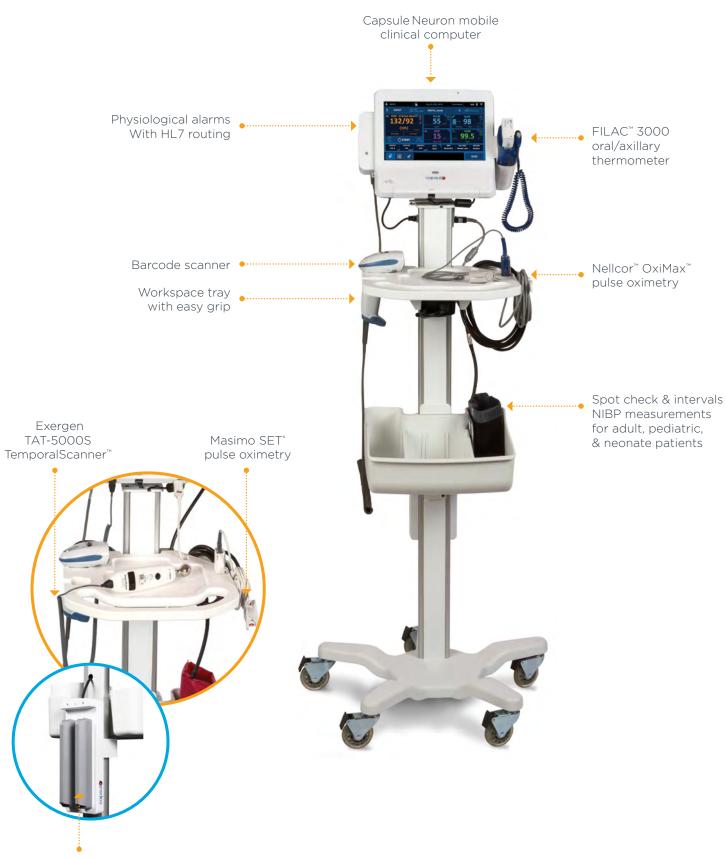

Hot-swappable batteries with 9.5-hour autonomy

SELECTED SPECIFICATIONS



Systolic Range Adult: 40 - 260 mmHg Pediatric: 40 - 230 mmHa Neonate: 40 - 130 mmHa Diastolic Range Adult: 20 - 200 mmHg Pediatric: 20 - 160 mmHg Neonate: 20 - 100 mmHg Adult: 26 - 220 mmHg MAP Range Pediatric: 26 - 183 mmHg Neonate: 26 - 110 mmHg

Clinical Accuracy ISO 81060-2:2013 for Adult, Pediatric, Neonate

Pulse Rate Range 30 to 220 bpm Pulse Rate Accuracy +2% or +3 bpm

Cuff Types SunTech Medical Reusable, Vinyl, Disposable

SpO₂

Masimo SET® (Signal Extraction Technology)**

SpO2 Range 1 - 100%

±2 digits for 70 - 100% Adult, Pediatric (No Motion) SpO2 Accuracy ±3 digits for 70 - 100% Adult, Pediatric (Motion)

±3 digits for 70 - 100% Neonate (No Motion, Motion)

Pulse Rate Range 25 - 240 bpm

±3 digits Adult, Pediatric, Neonate (No Motion) Pulse Rate Accuracy

±5 digits Adult, Pediatric, Neonate (Motion)

Perfusion Index 0.02% - 20%

Low Perfusion Performance ±2 digits for SpO2, ±3 digits for Pulse Rate (> 0.02% Pulse Amplitude and % Transmission > 5%)

Sensor Types Masimo LNCS Reusable and Single Patient Use

Nellcor™ OxiMax™ Technology

SpO2 Range 1 - 100%

SpO2 Accuracy*** ±2 digits for 70% - 100% Adult, Pediatric

±2 digits for 70% - 100% Neonate

±3 digits for 60% - 80% Adult, Pediatric, Neonate Low Sat

±2 digits for 70% - 100% Low Perfusion

±3 digits for 70% - 100% Adult, Pediatric, and Neonate with Motion

Pulse Rate Range 20 - 250 bpm

Pulse Rate Accuracy ±3 digits Adult, Pediatric, Neonate

±3 digits Low Perfusion

±5 digits (48 - 127 bpm) Adult, Pediatric, Neonate with Motion

Perfusion Index 0.03% - 20%

Sensor Types Nellcor™ OxiMax™ Reusable and Single Patient Use

Temperature

FILAC™ 3000 Thermometer+

35 to 43 °C (95 to 109 °F) Predictive Mode Temperature Range Clinical Accuracy ±0.2 °C (± 0.4 °F) difference between

Predictive and Direct Modes on 98% of

tested patients, meeting EN 12470-3

Response Time

Exergen TAT-5000S TemporalScanner™

15.5 to 43 °C (60 to 110 °F) Temperature Range

+/- 0.1 deg C (+/1 0.2 deg F) per ASTM E1112 Clinical Accuracy

capsule

** Masimo SET is clinically proven in over 100 studies as the superior pulse oximetry technology for its

ability to accurately measure during motion and low perfusion. SpO2 and Pulse Rate Accuracy

figures reflect use with LNCS finger sensors.

***Saturation accuracy varies by sensor type

pulse-oximetry

Refer to the "Sensor Accuracy Grid available

at www.medtronic.com/covidien/en-us/products/

Response Time ~0.04 seconds

6 - 10 seconds (oral), 8 - 12 seconds (axillary), + Functionality based on proprietary technology

of Cardinal Health Inc. 10 - 14 seconds (rectal) Predictive Mode

Scale Connectivity

Models Scale-Tronix® 4802, 5XX2, 6XX2, 51X5, 51X7, 6154

Method Automatic detection and capture via RS-232 Seca® 264, 284, 374, 486, 634, 664, 703, 704

Automatic detection and capture via 456 wireless dongle

Technical Characteristics

Operating Conditions 10 to 40°C (16 to 40°C with Exergen), 15 to 95% Humidity

-20 to 50°C, 15 to 90% Humidity Storage Conditions Ingress Protection IP31, except IPX0 with Exergen

Up to 9.5 hours with measurements every 10 minutes using hot swappable Dual Battery Dock Battery Autonomy

External Power Supply 100-240V AC, 2.0-1.0A, 50-60 Hz

Height: 1470 mm (57.9") x Width: 550 mm (21.7") x Depth: 550 mm (21.7") Dimensions

18 kg (39.7 lb) with Dual Battery Dock and roll stand Weight Network Connectivity 10/100/1000 base-T LAN WLAN IEEE 802.11 a/b/g/n Data Storage Capacity Saved/cached data sets persist for 72 hours

FOR MORE INFORMATION, CONTACT US

NORTH AMERICA

INTERNATIONAL OFFICES

+1800-260-9537 +33 1 84 17 12 50

international@capsuletech.com support@capsuletech.com

→ Learn more at CapsuleTech.com

CapsuleTech.com

MKT0264 DCN 2019-071 Rev 1.0 Published 2019-Apr